

# **3. Bioelectric Phenomena**

## **3-2 Hodgkin-Huxley Model**


### **Ion Channels**

### **Recent Tools**




# Hodgkin-Huxley model of the Action Potential

- An action potential does not decrease in amplitude as it is conducted away from its site of initiation. (**all or none**)
- An action potential occurs when  $V_m$  reaches the threshold potential at the axon hillock.



- Once  $V_m$  reaches threshold, **time- and voltage-dependent conductance changes occur in the active  $\text{Na}^+$  and  $\text{K}^+$  gates that drive  $V_m$  toward  $E_{\text{Na}}$ , then back to  $E_{\text{K}}$ , and finally to the resting potential.**



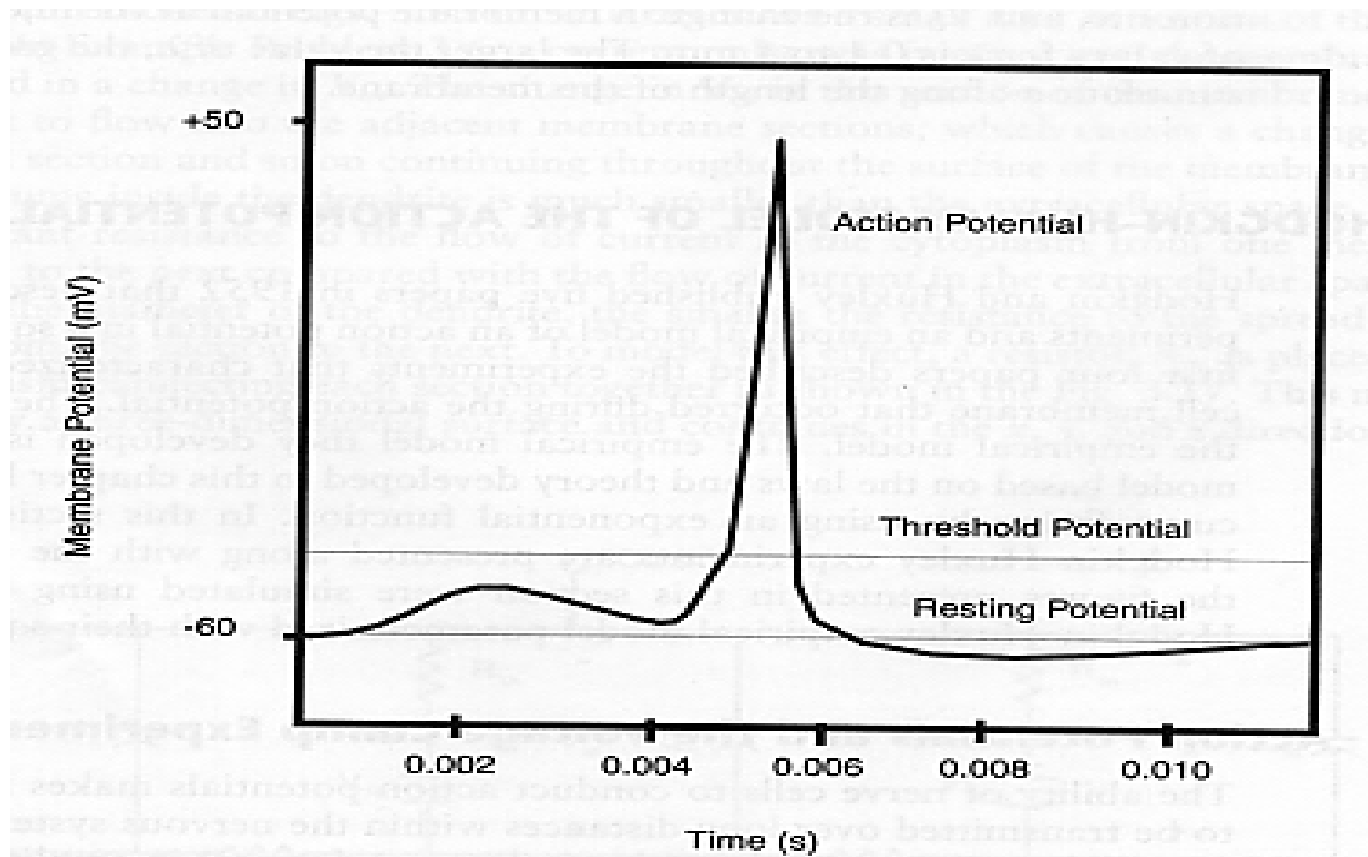

**Stylized diagram of an action potential once threshold potential is reached at approximately 5 ms. The action potential is due to voltage- and time-dependent changes in conductance. **The action potential rise is due to Na<sup>+</sup> and the fall is due to K<sup>+</sup> conductance change.****



- The action potential moves through the axon at high speeds and appears to **jump** from one Node of Ranvier to the next in myelinated neurons. (**Saltatory Conduction**)
- This occurs because the membrane capacitance of the myelin sheath is very small, making the membrane appear only **resistive** with almost instantaneous changes in  $V_m$  possible.
- To investigate the action potential, Hodgkin and Huxley used an unmyelinated **squid giant axon** in their studies because of its large diameter and long survival time of several hours in seawater at  $6.3^\circ\text{C}$




# Voltage Clamp

- The problem: two dynamic mechanisms in the channel during action potential: **time and voltage**
- Hodgkin and Huxley's contribution: **set voltage constant and obtain the time dependent changes of ionic currents** during action potential
- Method: Remove space variable(**space clamp**) and voltage variable(**voltage clamp**) by inserting long inner electrode and setting transmembrane-voltage constant by feedback.
- Two active channels are studied:  $K^+$  and  $Na^+$  channels
- Separation of  $K^+$  and  $Na^+$  channels was done by selection of external solution.
- 



# Voltage clamping

- Let displacement current 0  
 $I = C(dV/dt) = 0$   
 By forcing a constant voltage,



Give feedback using a Potentiostat to make


$$E_i - (E_o + E_c) = 0, \text{ then}$$

$E_i - E_o = E_c$ : voltage clamping



$E_i, E_o$ : membrane potential

$E_c$  : control voltage


Then the current  $E_o/R$  is the current injected to maintain constant  $V_m (= E_i - E_o)$ .



Voltage-clamp circuit for use with squid axon. a, axon; g, plastic guards. Uninsulated portion of internal voltage electrode indicated by short heavy line; uninsulated portion of current-injecting electrode indicated by long heavy line.  $E_i$ , internal potential;  $E_o$ , external potential;  $E_c$ , command potential. Feedback tends to make  $E_i - E_o = E_c$ . Injected current,  $I$ , measured as voltage drop across series resistor  $R$ .



$I$  : transmembrane current flowing to ground




-The initial pulse is the displacement current through capacitor due to the step increase in voltage

- the leakage current through passive gates:  $I_i = \frac{V_c - E_l}{R_l}$

This can be obtained by measuring the transmembrane current at below threshold (before activation of Na and K active gates)

- Subtracting both the capacitive and leakage current from  $I_m$  leaves only the Na<sup>+</sup> and K<sup>+</sup> currents.

To separate the Na<sup>+</sup> and K<sup>+</sup> currents, they chose a Na<sup>+</sup> free solution (they substituted a large impermeable cation for Na<sup>+</sup>).



(The results after subtractions) Diagram illustrating sodium and potassium currents due to a -20mV voltage clamp

(inward current is positive)







then to get G

$$I_K = \frac{V_m - E_K}{R_K} = G_K (V_m - E_K)$$
$$I_{Na} = \frac{V_m - E_{Na}}{R_{Na}} = G_{Na} (V_m - E_{Na})$$

- For all clamp voltage above threshold, the rate of onset for opening **Na<sup>+</sup> channel is more rapid** than for K<sup>+</sup> channels, and the Na<sup>+</sup> channels close after a period of time while K<sup>+</sup> channels remain open while the voltage clamp is maintained.
- Once the Na<sup>+</sup> channels close, they cannot be opened until the membrane has been hyperpolarized to its resting potential. The time spent in the closed state is called the **refractory period**.



# Normal vs. Na free solution



They did it for many voltages

(inward current is negative)



Intro. To BME

# The independent Na<sup>+</sup> and K<sup>+</sup> channels

- From the Voltage clamp:  
“The ionic current is divided into the initial Na<sup>+</sup> influx and the later K<sup>+</sup> outflux and these are independent.”
- Later, these have been verified through experiments using toxins: tetrodotoxin(TTX)(Na block) and tetraethylammonium(TEA)(K block)



# Equations Describing $G_{Na}$ and $G_K$

## The Differential Rate Equations

$$(1-m) \xrightleftharpoons[\beta_m]{\alpha_m} (m) \quad \frac{dm}{dt} = \alpha_m \cdot (1-m) - \beta_m \cdot m$$

$$(1-h) \xrightleftharpoons[\beta_h]{\alpha_h} (h) \quad \frac{dh}{dt} = \alpha_h \cdot (1-h) - \beta_h \cdot h$$

$$(1-n) \xrightleftharpoons[\beta_n]{\alpha_n} (n) \quad \frac{dn}{dt} = \alpha_n \cdot (1-n) - \beta_n \cdot n$$

$$h(t) = h_\infty - (h_\infty - h_0) \cdot e^{-t/\tau_h}$$

- $\alpha, \beta$  : gate open or close rate

$m, h, n$  are the fraction of open gates and  $(1-m), (1-h), (1-n)$  are fraction of closed gates.



- The rate constants  $\alpha$  and  $\beta$  are solely functions of voltage and change instantaneously with any change in voltage.
- The gating parameters  $m$ ,  $h$ , and  $n$  will change along exponential time courses. For example, the inactivation gates,  $h$ , will respond according to:

$$h(t) = h_s - (h_s - h_0) \exp(-t/\tau_h)$$

Here  $h_s$  is the steady-state value of  $h$  at the new voltage and  $h_0$  is the steady-state value of  $h$  prior to the voltage-step.  $\tau_h$  is the exponential time constant.



To explain the sigmoidal (Sshaped) kinetics of the rising phase of the sodium and potassium currents, Hodgkin and Huxley proposed that the Na channels were controlled by three activation (m) gates and the K channels were controlled by four activation (n) gates. By fitting the time courses of the Na and K conductances in response to voltage-clamp step changes in membrane voltage, Hodgkin and Huxley were able to obtain the values for the rate constants at different voltages from the following relations:

- Potassium

$$G_K = \bar{G}_K n^4$$


Sodium

$$G_{Na} = \bar{G}_{Na} m^3 h$$

i.e., maximum channel conductance multiplied by rate constants.




# Hodgkin Huxley model



## Circuit model and Equation for the Time Dependence of the Membrane Potential

$$I_m = G_K(V_m - E_K) + G_{Na}(V_m - E_{Na}) + \frac{(V_m - E_l)}{R_l} + C_m \frac{dV_m}{dt}$$

( $G_K$  and  $G_{Na}$ : the voltage-time-dependent conductance)

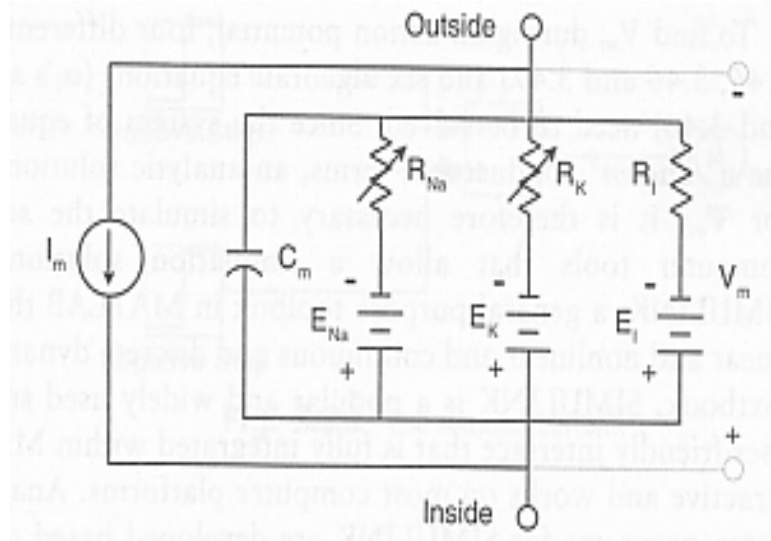

Circuit model of an unmyelinated section of squid giant axon..





- **We need to solve all differential equations regarding  $n$ ,  $m$  and  $h$  including algebraic expression for alphas and betas.**
- **Analytic solution is not possible due to the nonlinear nature of  $n$  and  $m$ .**
- **Simulation is necessary**
- **APSIM is a VB (virtual basic) based software that simulates action potentials. It uses a simple finite difference approximation to solve the series of differential equations.**




# Ion Channels



◆ Recent efforts to study Ion channels

1. Hodgkin–Huxley Model(1952)
2. Discovery of Channel Blockers(1965~1975)
3. Patch–clamping (1981) revealed functional characteristics of various ion channels
4. Some of the molecular structures were made known by molecular biology and genetic technologies(late 1990's)
5. Channel staining in Immune cell chemistry helped locate the ion channels.(2000's)






From Ion Channels of Excitable Membranes, third edition, by Bertil Hille, Sinauer, 2001

1975: after pharmacology and biophysics experiments:

**Fig. 3.6 Early Cartoon of a Voltage-Gated Channel**  
 The channel is drawn as a transmembrane protein with a hole through the center and is labeled with terms in use in 1975. The functional regions – **gate, voltage sensor, vestibules, and selectivity filter** – were deduced from voltage-clamp experiments. This diagram was drawn with results from Na channels in mind. [From Hille 1977c.]





After gene array test and protein analysis, they learned that a long protein constitutes a channel. The chain penetrates membrane at least 24 times for Na or Ca channels. Four small loops act as selectivity filter for a specific ion.


**Fig. 3.14 A 1991 Working Hypothesis for a Channel**

Fifteen years after Figure 3.6 was drawn, we had learned that there is significant channel mass in the intracellular and extracellular spaces; that there are four alpha-helical segments with positively charged residues acting as voltage sensors; and that channels are heavily glycosylated and tied to other intracellular proteins. [From Hille 1992.]







(A) Na CHANNEL



(B) Ca CHANNEL




(C) ONE QUARTER OF A K CHANNEL



This diagram shows the four loop filters. More important, it shows alpha and beta peptide chains. The Alpha-Peptide chain penetrates the membrane 24 times. They are grouped into four subunits numbered I/II/III/IV. Each group consists of 6 segments S1/S2/S3/S4/S5/S6. Among these S4 is the voltage sensor.






Voltage-gated channel의 S4 segment는 Voltage sensor의 많은 Gating charge를 운반한다. 이들은 Membrane potential의 변화에 반응해서 물리적으로 형태가 변화한다. Positive한 이들 Gating charge들은 Negative potential에서 세포 내부의 용액과 접촉하고 Positive potential에서는 외부의 용액과 접촉한다.

S1, S2, S3, S4로 구성되는 전체를 Voltage-sensing module이라고 하며, Channel이라 함은 이들 4개의 Transmembrane segment와 S5, S6 2개의 Transmembrane segment, 그리고 Core pore-forming complex인 P-loop를 말한다. S4가 주요 Voltage sensor이고 나머지 Module들은 선택적으로 세포 내, 외부로의 노출을 돕는 역할을 하는 정도라고 볼 수 있다.

### Plate 7. Models for opening of a voltage-gated channel.

The model shows two of the four subunits of a K channel, each with its six transmembrane helices (cylinders S1 to S6). The S4 segments are red and their gating charges yellow. The narrow selectivity filter formed by P-loops is not shown. (A) The channel is closed by the S6 segments crossed at the inner end. In a closed channel, the gating charge is mostly exposed to the inner solution via the internal crevice (arrow). (B) During a depolarization, the S4 segments rotate and the gating charges shift into the external crevice (arrow). This motion also favors a movement of the S5 and S6 segments that opens the pore. Because of the crevices in this model, a rotation of S4 suffices for voltage sensing without any outward movement. [After Cha, Snyder et al. 1999.]





Myelination은 Na, K Channel을 새롭게 분포시키는데(Rasband and Shrager 2000), Na Channel은 Node of Ranvier에 집중적으로 분포한다. Myelin이 없는 경우보다  $I_{Na}$  peak값이 10~15배에 이르고 Resting 상태에서의 Conduction도 10~100배에 이른다. K Channel도 Myelin으로 부분적으로 덮여있는 Node 주위에 많이 분포한다. Internode에는 대부분이 다양한 종류의 K Channel이고 Na Channel은 군데 군데 있는 정도이다. 이렇게 Node에 Channel들이 모여있는 것은 Protein scaffold, cytoskeletal elements, 복잡한 membrane protein들 때문이다. Plate 1은 Immunocytochemical 연구를 통해 얻은 것이다.






# more on the Neural Recordings



# Intracellular recording

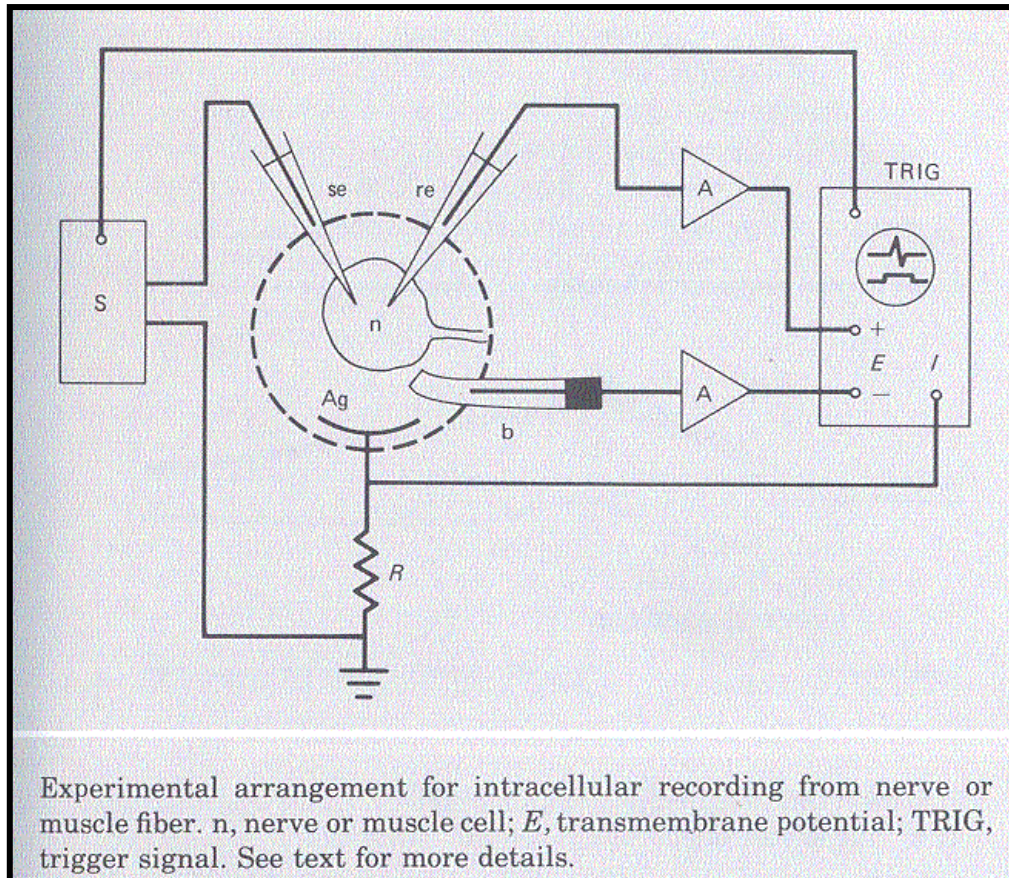


- High  $Z_{in}$  ( $10^{10}\Omega$ ), low gain DC Amp is needed.
  - Cf. high gain AC Amp is for extracellular work.

Figure 12






# Extracellular recording: Biphasic AP using bipolar electrodes.




A typical extracellular recording setup. Stimulus and recording. Conduction delay can also be considered.







# Monophasic AP recorded using killed-end recording.



Killed-end: always charged to + and unchanged.





# Compound AP and individual AP's separated in time.

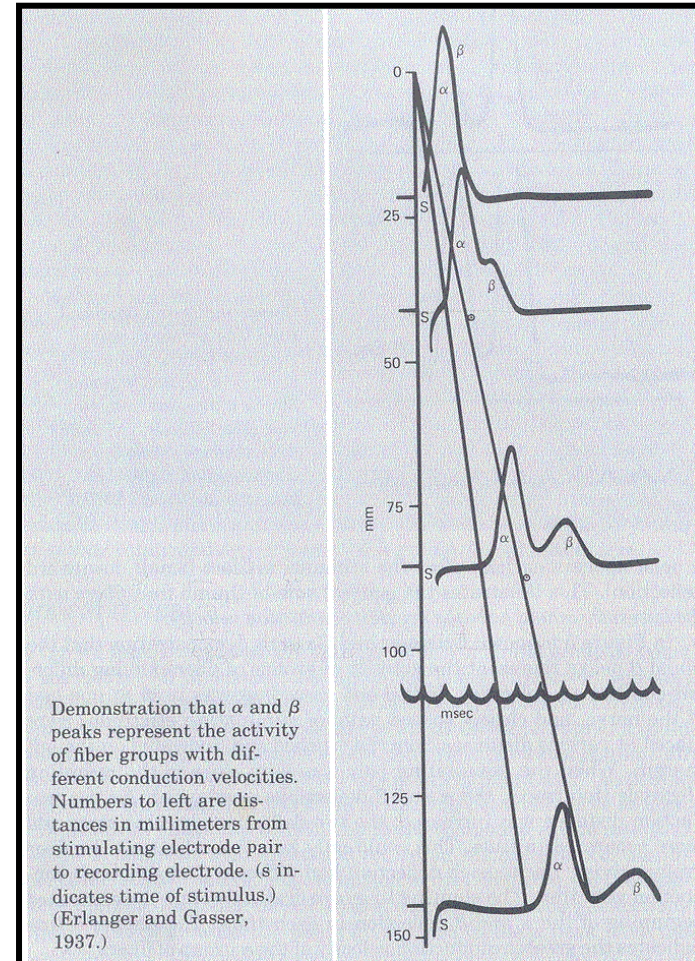






# Myelinated nerve, the node of Ranvier, Saltatory conduction.

- Very little current for the segments with myelinated sheath
- Almost no depolarization during the myelinated segment (potential is decremental)
- The non-decremental A.P. jumps over to next Ranvier node. (Saltatory conduction)
- Found in humans and higher animals.

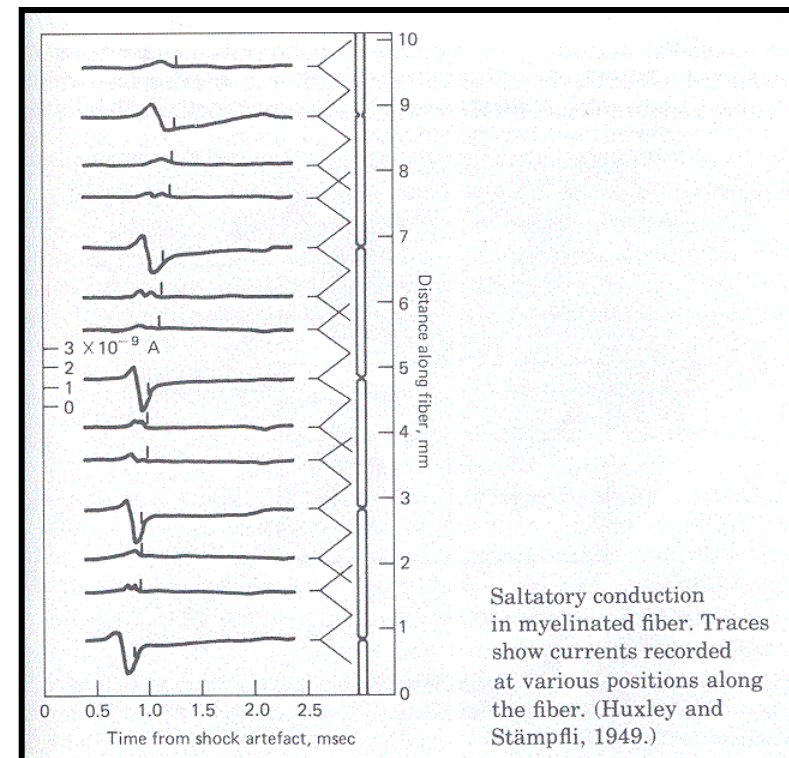

# Examples of Neural Recording Devices: MEA(MicroElectrode Array)



“Slant” Array

- This is a silicon based array of 100 penetrating microelectrodes, designed to be implanted in the cerebral cortex. It provides a means to stimulate and/or record from large number of neurons simultaneously.

- This is a variant of the UEA and contains 100 penetrating microelectrodes of various lengths (typically from 0.5 mm to 1.5 mm in length). The USA is designed to be implanted in the peripheral nervous system and to provide a means for simultaneous stimulation and recording from large number of nerve fibers.




Chronic Connector




# SNU Depth Probe

(A)



(B)




(C)




- A) Released whole wafer image,
- B) Fabricated 1 shank neural probe
- C) SEM Image - electrode sites and probe tip

# Neural Network Research with Planar Microelectrode Array




poly-l-lysine  
(containing FITC)  
Microstamped MEA

SNU Cult:  
Culture Plate  
type MEA



Culture Plate



Cultured hippocampal  
neurons In low density

